
LNB0401-060-P C13H17NO MW=203

University of Birmingham, School of Chemistry
Waters Xevo G2-XS

Daniel Kovari
11-Dec-2020 15:40:31

LRC-DXK-3UTEV-ASAP-Pos-2 169 (3.349) AM2 (Ar,22000.0,0.00,0.00); ABS

1: TOF MS ASAP+
2.42e6

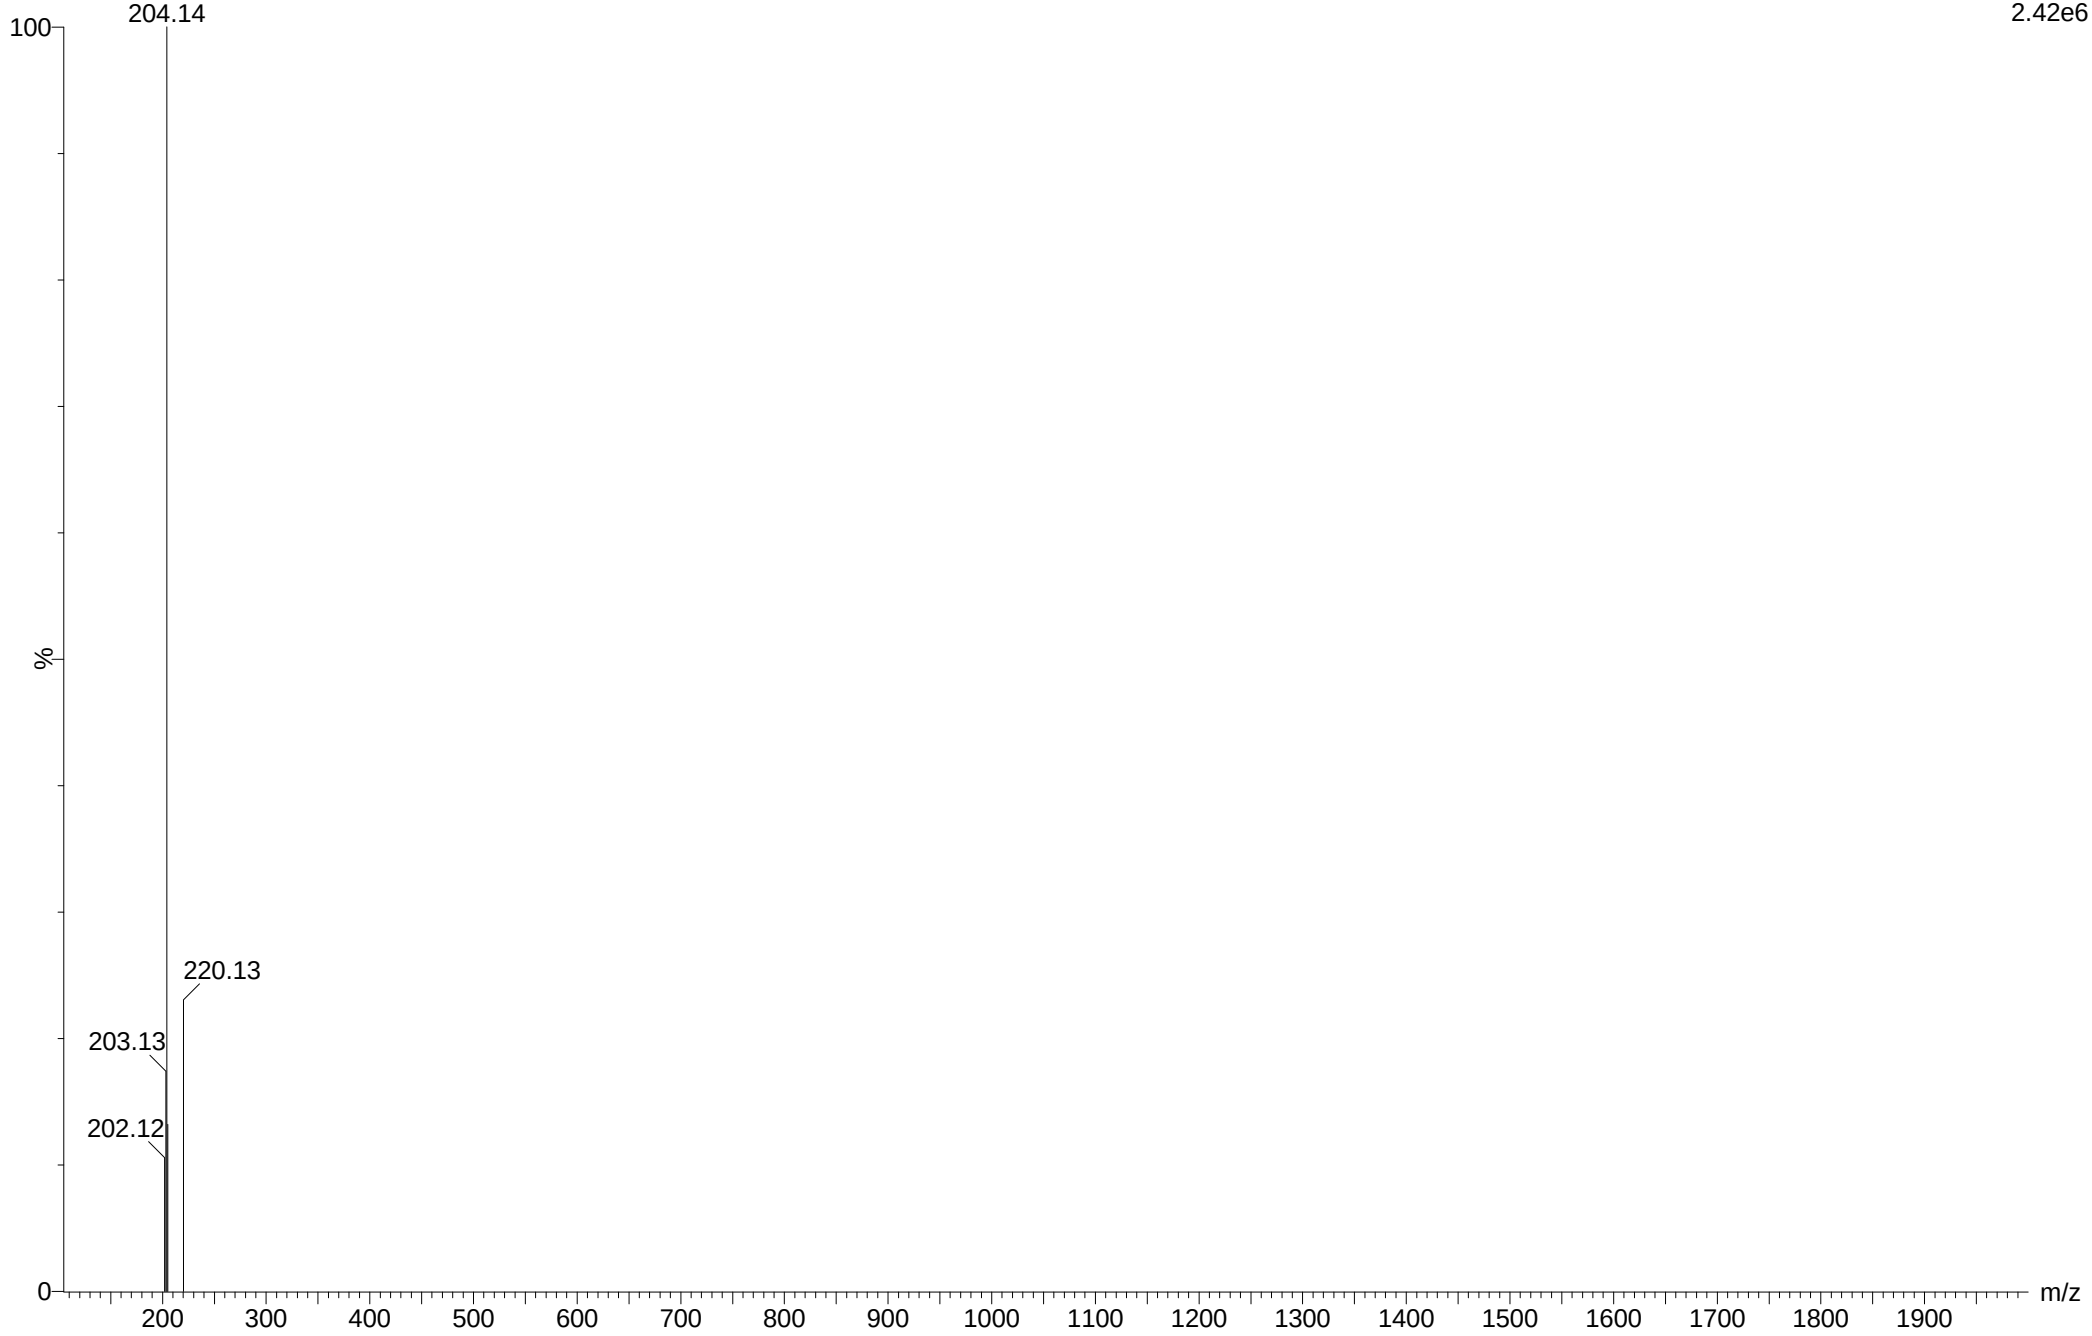


LNB0401-060-P C13H17NO MW=203

University of Birmingham, School of Chemistry
Waters Xevo G2-XS

Daniel Kovari
11-Dec-2020 15:40:31


LRC-DXK-3UTEV-ASAP-Pos-2 (0.070) Is (1.00,0.01) C13H17NO

1: TOF MS ASAP+
8.63e12

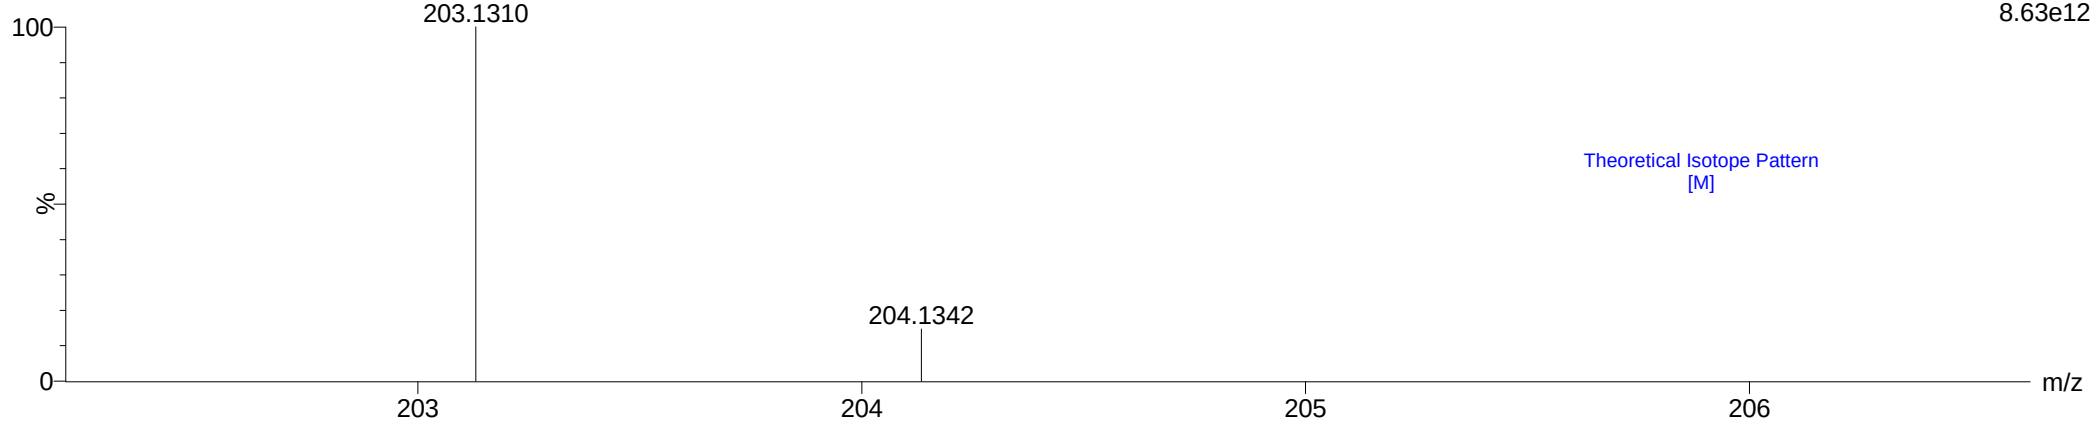


LRC-DXK-3UTEV-ASAP-Pos-2 (0.070) Is (1.00,0.01) C13H17NO H

1: TOF MS ASAP+
8.62e12

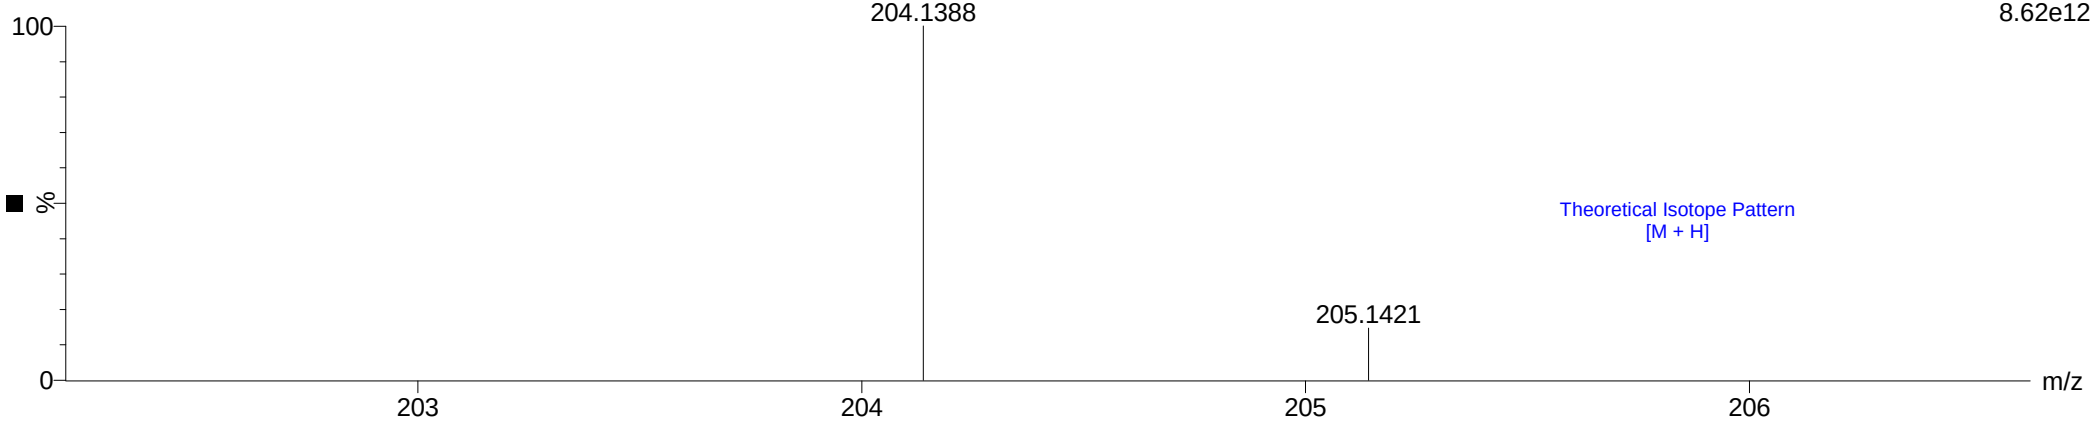

LRC-DXK-3UTEV-ASAP-Pos-2 169 (3.349) AM2 (Ar,22000.0,0.00,0.00); ABS

1: TOF MS ASAP+
2.42e6

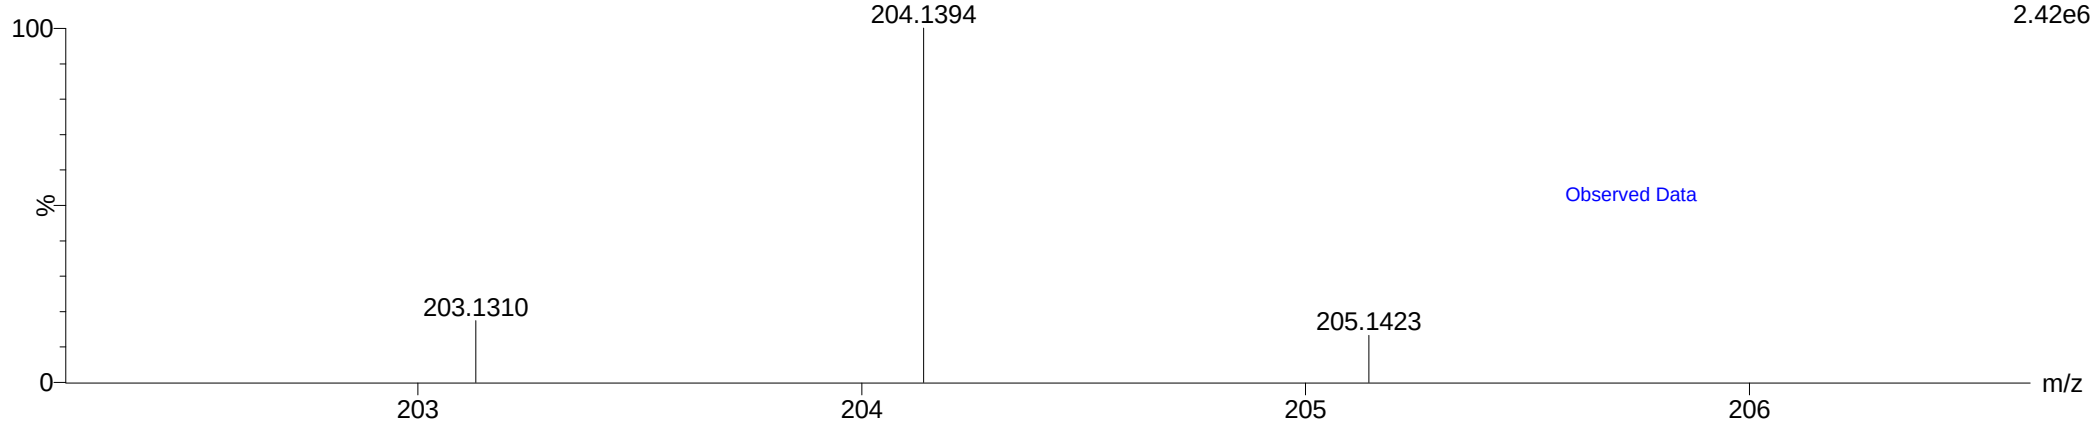


LNB0401-060-P C13H17NO MW=203

University of Birmingham, School of Chemistry
Waters Xevo G2-XS

Daniel Kovari
11-Dec-2020 15:40:31


LRC-DXK-3UTEV-ASAP-Pos-2 (0.070) Is (1.00,0.01) C13H17NO H

1: TOF MS ASAP+
8.62e12

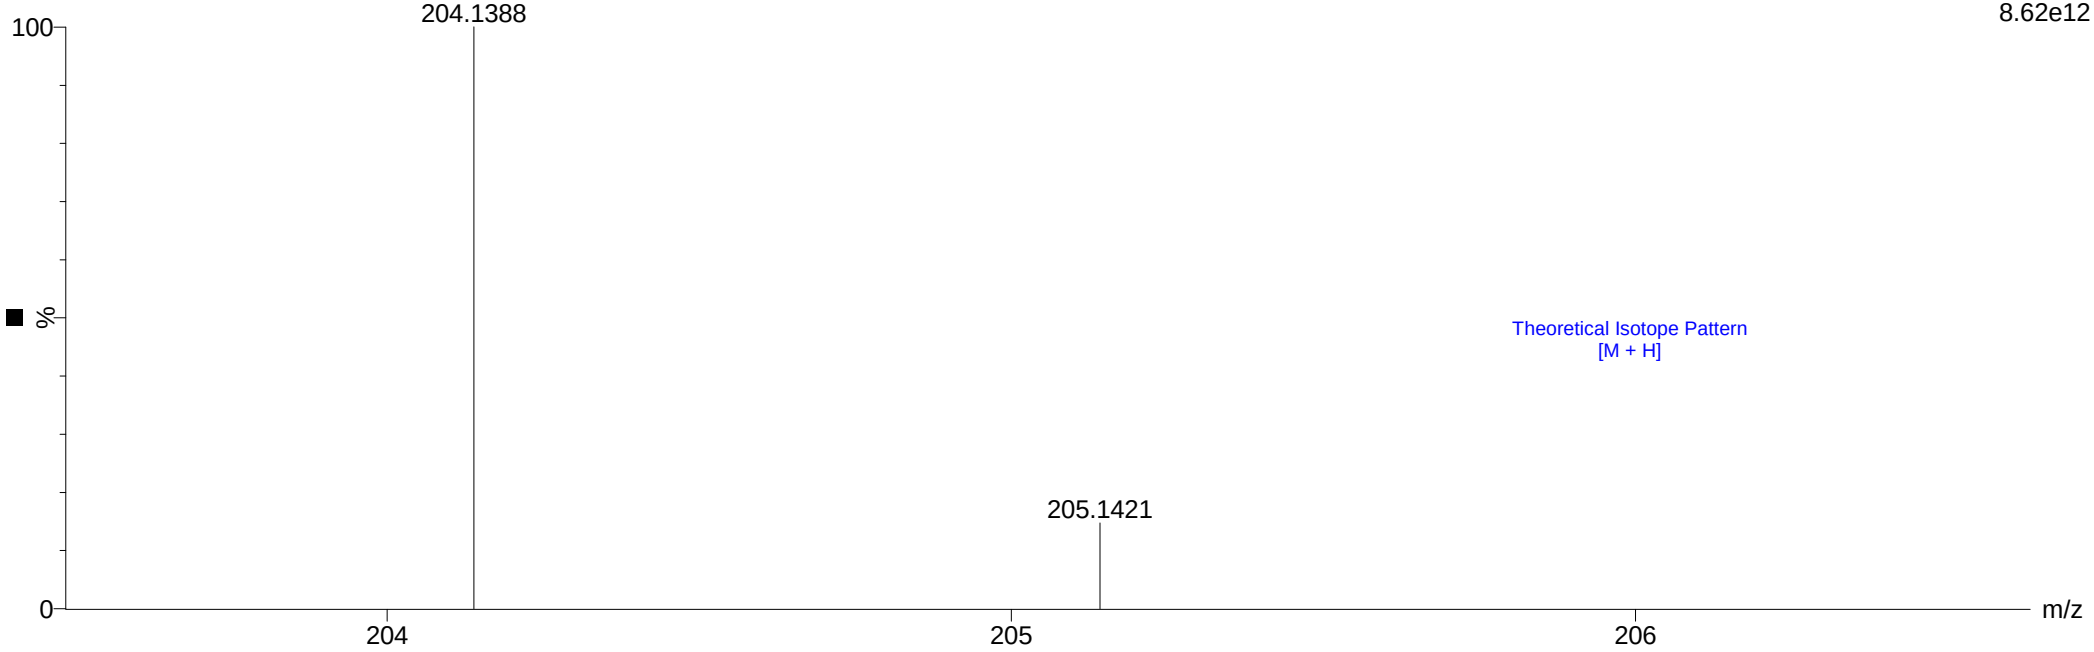

LRC-DXK-3UTEV-ASAP-Pos-2 169 (3.349) AM2 (Ar,22000.0,0.00,0.00); ABS

1: TOF MS ASAP+
2.42e6

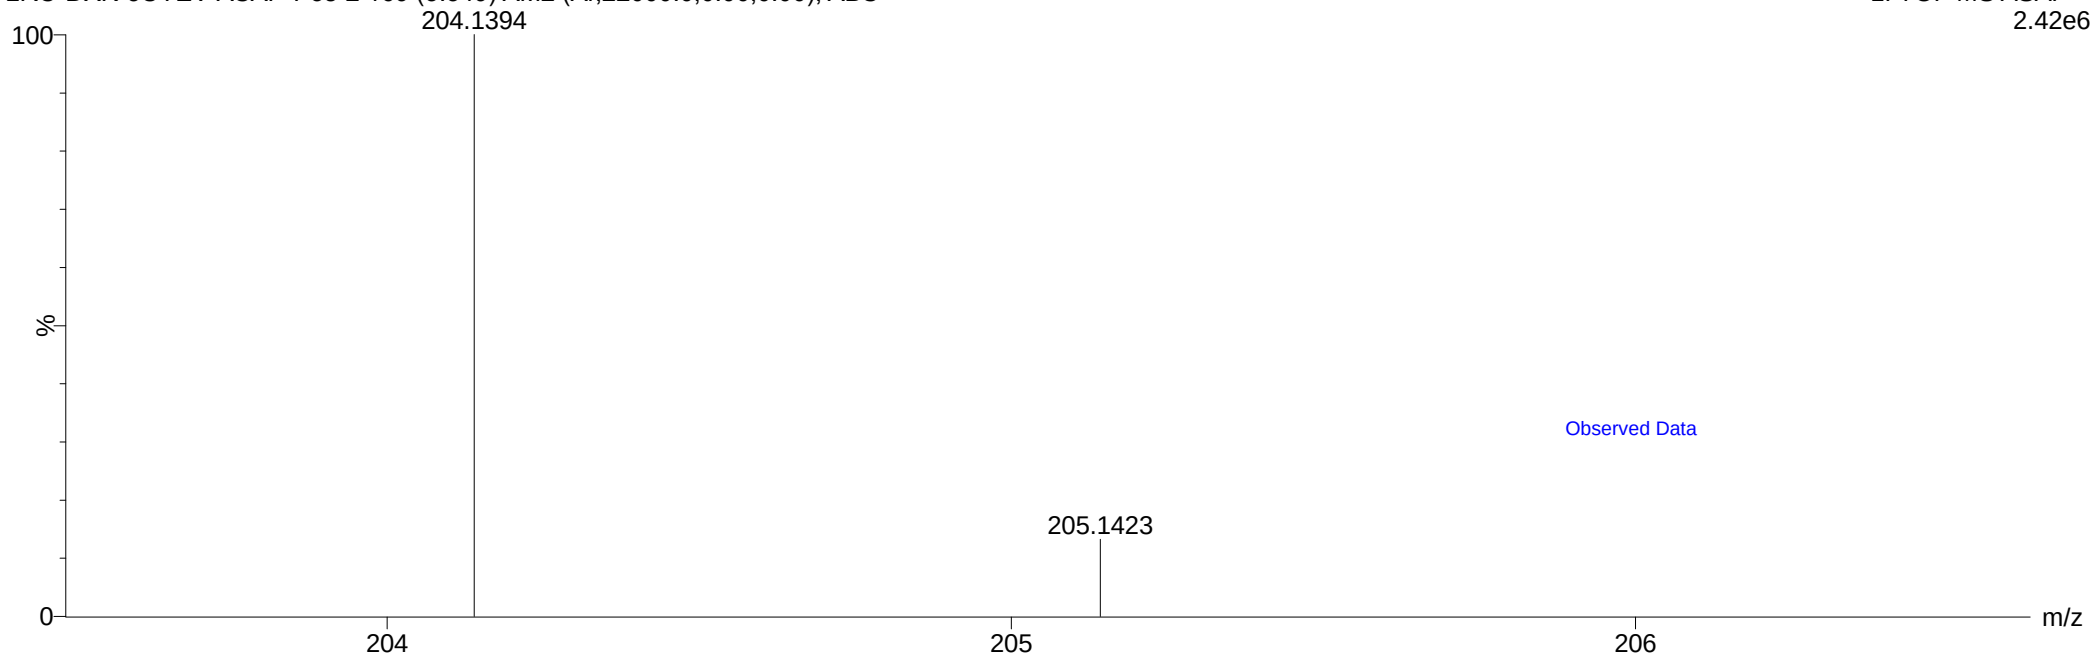

Single Mass Analysis

Tolerance = 3.0 PPM / DBE: min = -10.0, max = 100.0
Element prediction: Off
Number of isotope peaks used for i-FIT = 4

Monoisotopic Mass, Even Electron Ions
307 formula(e) evaluated with 1 results within limits (all results (up to 1000) for each mass)
Elements Used:
C: 0-50 H: 0-60 N: 0-10 O: 0-10

Minimum:				-10.0				
Maximum:		5.0	3.0	100.0				
Mass	Calc. Mass	mDa	PPM	DBE	i-FIT	Norm	Conf(%)	Formula
204.1394	204.1388	0.6	2.9	5.5	48.8	n/a	n/a	C13 H18 N O