

HS_05dec2022 on NEO500



Current Data Parameters
NAME HS_05dec2022
EXPNO 11
PROCNO 1


F2 - Acquisition Parameters
Date_ 20221208
Time 3.09 h
INSTRUM CAB AV4 500 MHz BASIC
PROBHD Z150364_0007 (
PULPROG noesygpph
TD 2048
SOLVENT CD3CN
NS 32
DS 16
SWH 4716.981 Hz
FIDRES 4.606427 Hz
AQ 0.2170880 sec
RG 28.5
DW 106.000 usec
DE 45.36 usec
TE 298.0 K
D0 0.00009072 sec
D1 1.95494401 sec
D8 0.50000000 sec
D11 0.03000000 sec
D12 0.00002000 sec
D16 0.00020000 sec
IN0 0.00021200 sec
TDav 1
SF01 500.0758585 MHz
NUC1 1H
P1 12.00 usec
P2 24.00 usec
P17 2500.00 usec
PLW1 14.55099964 W
PLW10 2.32820010 W
GPNAM[1] SMSQ10.100
GPZ1 40.00 %
P16 1000.00 usec

===== F1 INDIRECT DIMENSION =====
td1 440
sw_F1 9.432531

F1 - Acquisition parameters
TD 440
SF01 500.0759 MHz
FIDRES 21.440823 Hz
SW 9.433 ppm
FnMODE States-TPPI

F2 - Processing parameters
SI 2048
SF 500.0730000 MHz
WDW QSINE
SSB 2
LB 0 Hz
GB 0
PC 1.40

F1 - Processing parameters
SI 1024
MC2 States-TPPI
SF 500.0730000 MHz
WDW QSINE
SSB 2
LB 0 Hz
GB 0

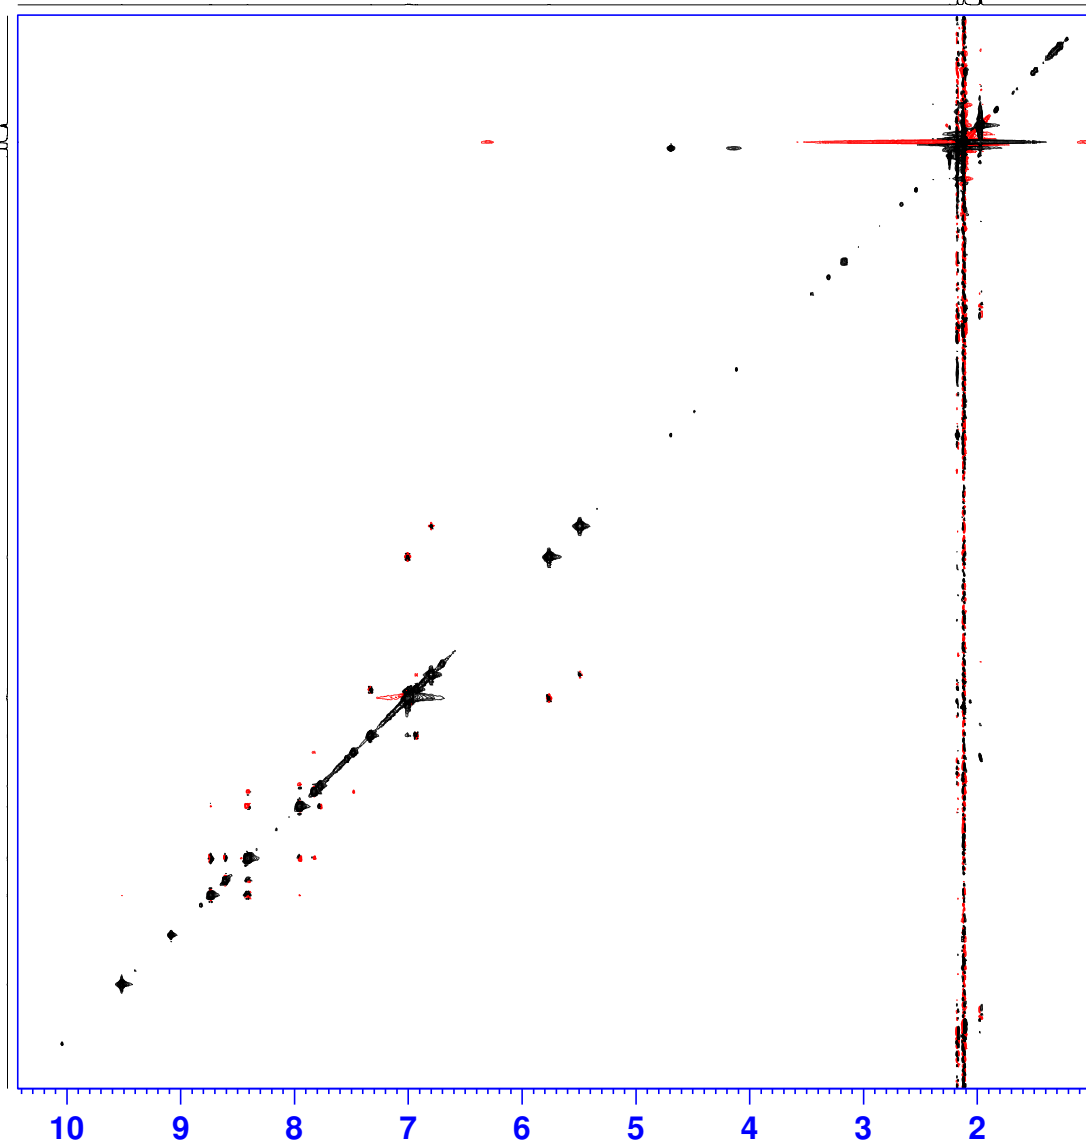

ppm

2

3

4

5

6

7

8

9

10

ppm